



## Free T3 EIA Test Kit Package Insert

REF	I231-3051	English
-----	-----------	---------

An enzyme immunoassay (EIA) for the *in vitro* quantitative detection of Free T3 (Triiodothyronine) in human serum.

For professional *in vitro* diagnostic use only.

### INTENDED USE

The Free T3 EIA Test Kit is an enzyme immunoassay for the *in vitro* quantitative detection of Free T3 (Triiodothyronine) in human serum.

### SUMMARY

3,5,3' Triiodothyronine (T3) is a thyroid hormone with a molecular weight of 651 daltons.<sup>1</sup> About 20 percent of the body's T3 comes from the synthesis of T3 within the thyroid while the rest is derived by deiodination of the other thyroid hormone thyroxine (T4) which occurs in the peripheral tissues.<sup>2,3</sup> Although T3 is present in less concentration than T4, it is more rapid and biologically active. T3 is bound to thyroxine binding globulin (TBG), prealbumin and albumin in blood. Approximately 0.3% is present unbound or free T3 and represents the physiologically active thyroid hormone. While Total T3 concentrations are dependent on thyroid status, peripheral conversion of T4 to T3, or on the level of TBG during many clinical conditions such as pregnancy and administration of oral contraceptives, Free T4 is less sensitive and remains constant. Therefore, free T3 may provide better indication of thyroid status. Measurement of Free T3 is generally recommended for hyperthyroidism found in Graves' disease and toxic adenomas.<sup>4,5</sup> The Free T3 EIA Test Kit is an immunoassay for the quantitative detection of the presence of Free T3 (Triiodothyronine) in serum specimen. The test utilizes monoclonal antibodies to selectively detect Free T3 in serum

### PRINCIPLE

The Free T3 EIA Test Kit is a solid phase enzyme immunoassay based on a competitive principle for the quantitative detection of Free T3 in human serum. The microwell plate is coated with a fixed amount of monoclonal antibodies specific to T3. During testing, the specimen along with T3 enzyme-conjugate are added to the antibody coated microwell plate and then incubated. If the specimen contains T3, it will compete with the T3 enzyme-conjugated to bind to the antibodies coated on the microwell plate. If the specimen does not contain T3, only the T3 enzyme-conjugate will bind to the inside of the plate. After initial incubation, the microwell plate is washed to remove unbound materials. Substrate A and substrate B are added and then incubated to produce a blue color, indicating the amount of T3 enzyme-conjugate bound to the plate. If Free T3 is present in the sample, it will block the antibody binding sites and when the substrate is added there will be no color development. The absence of color or low amount of color thus indicates the presence of Free T3 in the specimen. Sulfuric acid solution is added to the microwell plate to stop the reaction which produces a color change from blue to yellow. The color intensity, which is inversely proportional to the amount of Free T3 present in the specimen, is measured with a microplate reader at 450/630-700 nm or 450 nm. The absorbance of the specimen is then compared to a calibration curve to obtain the amount of Free T3 present in the specimen.

### PRECAUTIONS

- For professional *in vitro* diagnostic use only. Do not use after expiration date.
- Do not mix reagents from other kits with different lot numbers.
- Avoid cross contamination between reagents to ensure valid test results.
- Follow the wash procedure to ensure optimum assay performance.
- Use Plate Sealer to cover microwell plate during incubation to minimize evaporation.
- Use a new pipet tip for each specimen assayed.
- Ensure that the bottom of the plate is clean and dry and that no bubbles are present on the surface of the liquid before reading the plate. Do not allow wells to dry out during the assay procedure.
- Do not touch the bottom of the wells with pipette tips. Do not touch the bottom of the microwell plate with fingertips.
- Do not allow sodium hypochlorite fumes from chlorine bleach or other sources to contact the microwell plate during the assay as the color reaction may be inhibited.
- All equipment should be used with care, calibrated regularly and maintained following the equipment manufacturer's instructions.

### HEALTH AND SAFETY INFORMATION

- Some components of this kit contain human blood derivatives. These materials are tested as negative for antibody to HIV 1/2, antibody to HCV, HIV Ag, HIV NAT, HBsAg and Syphilis. No known test method can offer complete assurance that products derived from human blood will not transmit infectious agents. Therefore, all blood derivatives should be considered potentially infectious. It is recommended that these reagents and human specimens be handled using established good laboratory working practices.
- Wear disposable gloves and other protective clothing such as laboratory coats and eye protection while handling kit reagents and specimens. Wash hands thoroughly when finished.
- ProClin™ 300 is included as a preservative in the Conjugate Diluent, Concentrated Wash Buffer, Substrate and Calibrators. Avoid any contact with skin or eyes.
- Do not eat, drink or smoke in the area where the specimens or kits are handled. Do pipette by mouth.
- Avoid any contact of the Substrate and Stop Solution with skin or mucosa. The Stop Solution

contains 0.5 M sulfuric acid which is a strong acid. If spills occur, wipe immediately with large amounts of water. If the acid contacts the skin or eyes, flush with large amounts of water and seek medical attention.

- Non-disposable apparatus should be sterilized after use. The preferred method is to autoclave for one hour at 121°C. Disposables should be autoclaved or incinerated. Do not autoclave materials containing sodium hypochlorite.
- Handle and dispose all specimens and materials used to perform the test as if they contained infectious agents. Observe established precautions against microbiological hazards throughout all the procedures and follow the standard procedures for proper disposal of specimens.
- Observe Good Laboratory Practices when handling chemicals and potentially infectious material. Discard all contaminated material, specimens and reagents of human origin after proper decontamination and by following local, state and federal regulations.
- Neutralized acids and other liquids should be decontaminated by adding sufficient volume of sodium hypochlorite to obtain a final concentration of at least 1.0%. A 30 minute exposure to a 1.0% sodium hypochlorite may be necessary to ensure effective decontamination.

### STORAGE AND STABILITY

- Unopened test kits should be stored at 2-8°C upon receipt. All unopened reagents are stable through the expiration date printed on the box if stored between 2-8°C. Once opened, all reagents are stable for up to 3 months after the first opening date if stored between 2-8°C. Return reagents to 2-8°C immediately after use. Avoid freezing and thawing the kit. 3 freeze-thaw cycles may increase determined values.
- Allow the sealed pouch to reach room temperature before opening the pouch and remove the required number of strips to prevent condensation of the microwell plate. The remaining unused strips should be stored in the original resealable pouch with desiccant supplied at 2-8°C and can be used within 3 months of the opening date. Return the remaining unused strips and supplied desiccant to the original resealable pouch, firmly press the seal closure to seal the pouch completely and immediately store at 2-8°C.
- Concentrated Wash Buffer may be stored at room temperature to avoid crystallization. If crystals are present, warm up the solution at 37°C. Working Wash Buffer is stable for 2 weeks at room temperature.
- Do not expose reagents especially the Substrate to strong light or hypochlorite fumes during storage or incubation steps.
- Do not store Stop Solution in a shallow dish or return it to the original bottle after use.

### SPECIMEN COLLECTION AND PREPARATION

- The Free T3 EIA Test Kit can be performed using only human serum collected from venipuncture whole blood.
- The preservative sodium azide inactivates horseradish peroxidase and may lead to erroneous results.
- Separate serum from blood as soon as possible to avoid hemolysis. Grossly hemolytic, lipidic or turbid samples should not be used. Specimen with extensive particulate should be clarified by centrifugation prior to use. Do not use specimens with fibrin particles or contaminated with microbial growth.
- Serum specimens may be stored at 2-8°C for up to 7 days prior to assaying. For long term storage, specimens should be kept frozen below -20°C.
- Bring specimens to room temperature prior to testing. Frozen specimens must be completely thawed and mixed well prior to testing. Specimens should not be frozen and thawed repeatedly.
- If specimens are to be shipped, they should be packed in compliance with local regulations covering the transportation of etiologic agents.

### REAGENTS AND COMPONENTS

#### Materials Provided

No.	Reagent	Component Description	Quantity	
			96 wells/kit	480 wells/kit
	Free T3 Microwell Plate	Microwell plate coated with monoclonal Anti-T3	1 plate (96 wells/plate)	5 plates (96 wells/plate)
1	Concentrated Conjugate(11x)	Concentrated T3-HRP;	1 x 0.6 mL	5 x0.6 mL
1A	Conjugate Diluent	Tris-HCl buffer Preservative: 0.1% ProClin™ 300	1 x 6 mL	5 x 6 mL
2	Concentrated Wash Buffer (25x)	Tris-HCl buffer containing 0.1% Tween 20; Preservative: 0.1% ProClin™ 300	1 x 40 mL	5 x 40 mL
3	Substrate A	Citrate-phosphate buffer containing hydrogen peroxide; Preservative: 0.1% ProClin™ 300	1 x 8 mL	5 x 8 mL
4	Substrate B	Buffer containing tetramethylbenzidine (TMB); Preservative: 0.1% ProClin™ 300	1 x 8 mL	5 x 8 mL
5	Stop Solution	0.5 M Sulfuric acid	1 x 8 mL	5 x 8 mL

6	Free T3 Calibrator 1	Human serum without FreeT3; Preservative: 0.15% ProClin™ 300	1 x 0.5 mL	5 x 0.5 mL
7	Free T3 Calibrator 2		1 x 0.5 mL	5 x 0.5 mL
8	Free T3 Calibrator 3	Human serum containing a certain amount of Free T3 (pg/mL), the concentration is gradually increased from Calibrator 2 to Calibrator 6; Preservative: 0.15%ProClin™ 300	1 x0.5 mL	5 x 0.5 mL
9	Free T3 Calibrator 4		1 x 0.5 mL	5 x 0.5 mL
10	Free T3 Calibrator 5		1 x0.5 mL	5 x 0.5 mL
11	Free T3 Calibrator 6		1 x 0.5 mL	5 x 0.5 mL
	Plate Sealers		2	10
	Package Insert		1	1

#### Materials Required But Not Provided

- Freshly distilled or deionized water
- Sodium hypochlorite solution for decontamination
- Absorbent paper or paper towel
- Water bath or incubator capable of maintaining 37°C ± 2°C.
- Calibrated automatic or manual microwell plate washer capable of aspirating and dispensing 350 µL/well
- Disposable gloves
- Automated processor (optional)
- Calibrated micropipettes with disposable tips capable of dispensing 50 µL and 100 µL
- Graduated cylinders for wash buffer dilution
- Vortex mixer for specimen mixing (optional)
- Disposable reagent reservoirs
- Calibrated microplate reader capable of reading at 450 nm with a 630-700 nm reference filter, or reading at 450 nm without a reference filter
- Timer

### DIRECTIONS FOR USE

Allow reagents and specimens to reach room temperature (20-30°C) prior to testing. The procedure must be strictly followed. Assay must proceed to completion within time limits. Arrange the calibrators in a horizontal or vertical configuration. The procedure below assigns specific wells arranged in a vertical configuration. Configuration may depend upon software.

Step	Detailed Procedure	Simplified Procedure
	<ul style="list-style-type: none"> <li>Prepare Working Wash Buffer by diluting the Concentrated Wash Buffer 1:24 Pour the contents of the bottle containing the concentrated wash buffer in a graduated cylinder and fill it with freshly distilled or deionized water to 1000 mL for 96 wells/plate testing. The Working Wash Buffer is stable for 2 weeks at 15-30°C.</li> <li><b>Note:</b> If crystals are present in the Concentrated Wash Buffer, warm it up at 37°C until all crystals dissolve.</li> <li>Prepare Working Conjugate by diluting concentrated conjugate (11x) with conjugate Diluent 1:10. Fresh preparation is recommended. The Working conjugate should be stored at 2-8°C and used within 72 hours</li> <li><b>Note:</b> Conjugate diluent may have a little precipitation. Please mix well before use.</li> <li>Remove unused strips from the microwell plate, and store in the original resealable pouch at 2-8°C.</li> </ul>	<ul style="list-style-type: none"> <li>Prepare Working Wash Buffer by diluting the Concentrated Wash Buffer 1:24</li> <li>Prepare Working conjugate by diluting Anti-T3 (11x) with conjugate Diluent 1:10.</li> <li>Remove and store unused strips at 2-8°C</li> </ul>
0	• Leave A1 as Blank well.	• Leave A1 as Blank well.
1	<ul style="list-style-type: none"> <li>• Add 50 µL of Calibrator 1 in wells B1 and C1.</li> <li>• Add 50 µL of Calibrator 2 in wells D1 and E1.</li> <li>• Add 50 µL of Calibrator 3 in wells F1 and G1.</li> <li>• Add 50 µL of Calibrator 4 in wells H1 and A2.</li> <li>• Add 50 µL of Calibrator 5 in wells B2 and C2.</li> <li>• Add 50 µL of Calibrator 6 in wells D2 and E2.</li> </ul>	<ul style="list-style-type: none"> <li>• B1 and C1: Add 50 µL Calibrator 1</li> <li>• D1 and E1: Add 50 µL Calibrator 2</li> <li>• F1 and G1: Add 50 µL Calibrator 3</li> <li>• H1 and A2: Add 50 µL Calibrator 4</li> <li>• B2 and C2: Add 50 µL Calibrator 5</li> <li>• D2 and E2: Add 50 µL Calibrator 6</li> </ul>
2	• Add 50 µL of specimen to assigned wells starting at F2 and G2.	• Starting F2 and G2: Add 50 µL specimen
3	• Add 50 µL of Conjugate to each well except for the Blank well. (Red Reagent).	• Add 50 µL of Conjugate to each well
4	<ul style="list-style-type: none"> <li>• Mix gently by swirling the microwell plate on a flat bench for 30 seconds.</li> <li>• Cover the microwell plate with the Plate Sealer and incubate in a water bath or an incubator at 37°C for 60 minutes ± 2 minutes.</li> </ul>	<ul style="list-style-type: none"> <li>• Mix gently</li> <li>• Cover the microwell plate with the Plate Sealer and incubate at 37°C for 60 min</li> </ul>

5	<ul style="list-style-type: none"> <li>Remove the Plate Sealer.</li> <li>Wash each well 5 times with 350 µL of Working Wash Buffer per well, then remove the liquid.</li> <li>Turn the microwell plate upside down on absorbent tissue for a few seconds. Ensure that all wells have been completely washed and dried.</li> </ul> Note: Improper washing may cause false results.	<ul style="list-style-type: none"> <li>Remove the Plate Sealer</li> <li>Wash each well 5 times with 350 µL of Working Wash Buffer</li> <li>Turn the microwell plate upside down on absorbent tissue</li> </ul>
6	<ul style="list-style-type: none"> <li>Add 50 µL of Substrate A to each well. (Clear Reagent)</li> <li>Add 50 µL of Substrate B to each well. (Clear Reagent)</li> </ul> Then a blue to light blue color should develop in wells corresponding to the amount of Free T3 present in the specimen.	<ul style="list-style-type: none"> <li>Add 50 µL of Substrate A to each well</li> <li>Add 50 µL of Substrate B to each well</li> </ul>
7	<ul style="list-style-type: none"> <li>Mix gently then cover microwell plate with Plate Sealer and incubate in a water bath or incubator at room temperature (20-30°C) for 15 minutes ± 1 minute.</li> </ul>	<ul style="list-style-type: none"> <li>Mix then cover microwell plate with Plate Sealer and incubate at room temperature for 15 min</li> </ul>
8	<ul style="list-style-type: none"> <li>Remove the Plate Sealer.</li> <li>Add 50 µL of Stop Solution to each well. (Clear Reagent)</li> </ul> Then a yellow to light yellow color should develop in wells corresponding to the amount of Free T3 present in the specimen.	<ul style="list-style-type: none"> <li>Remove Plate Sealer</li> <li>Add 50 µL of Stop Solution to each well</li> </ul>
9	<ul style="list-style-type: none"> <li>Read at 450/630-700 nm within 30 minutes.</li> </ul> Note: Microwell plate can also be read at 450 nm, but it is strongly recommended to read it at 450/630-700 nm for better results.	<ul style="list-style-type: none"> <li>Read at 450/630-700 nm within 30 min</li> </ul>

#### AUTOMATED PROCESSING

Automatic EIA microplate processors may be used to perform the assay after validating the results to ensure they are equivalent to those obtained using the manual method for the same specimens. Incubation times may vary depending on the processors used but do not program less incubation times than the procedure listed above. When automatic EIA microplate processors are used, periodic validation is recommended to ensure proper results.


#### QUALITY CONTROL

Control standards are not supplied with this kit; however, it is recommended that low, normal and high controls be tested with each run as a good laboratory practice to monitor assay performance. Each laboratory should establish its own criteria for establishing mean values and acceptable ranges to determine reliability of the results.

#### CALCULATION OF RESULTS

Draw the calibration curve and obtain quantitative specimen results.

- Record the absorbance obtained from the printout of microplate reader as outlined in the Example of Specimen & Calibrators Result Calculation.
- Plot the absorbance for each duplicate reference versus the corresponding concentration in pg/mL on linear graph paper.
- Draw the best-fit curve through the plotted points.
- Determine the concentration of Free T3 for an unknown by locating the absorbance of specimen on the vertical axis of the graph, find the intersecting point on the curve, and read the concentration (in pg/mL) from the horizontal axis of the graph.

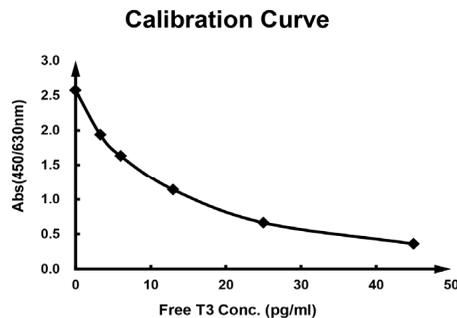

#### Example of Specimen & Calibrators Result Calculation

Item	Well	Absorbance	Mean (Absorbance – Blank)	Concentration (pg/mL)
Blank Well	A1	0.003	/	/
Calibrator 1	B1	2.628	2.572	0.0
	C1	2.521		
Calibrator 2	D1	1.944	1.933	3.3
	E1	1.927		

Calibrator	F1	1.609	1.627	6.0
		G1		
Calibrator 4	H1	1.212	1.135	13.0
		A2		
Calibrator 5	B2	0.648	0.660	25.0
		C2		
Calibrator 6	D2	0.379	0.358	45.0
		E2		
Unknown Specimen	F2	1.896	1.889	3.69
		G2		

#### LIMITATIONS

- The Free T3 EIA Test Kit is used for the detection of Free T3 in human serum. Diagnosis should not be established based on a single test result. Further testing should be performed in assessing clinical status. Specimens containing precipitate may give inconsistent test results.
- As with all diagnostic tests, all results must be interpreted together with other clinical information available to the physician.
- As with other sensitive immunoassays, there is the possibility that the positive result cannot be repeated due to inadequate washing from the initial test. The results may be affected due to procedural or instrument error.
- The Free T3 EIA Test Kit is not intended for use in screening of newborns.

#### EXPECTED VALUES

It is recommended that each laboratory establish its own range of expected values based on patient populations. The table below should be regarded as an initial reference only.

Population	No. Specimens	Mean (pg/mL)	Range (pg/mL)
Normal	75	3.47	1.97-4.98

#### PERFORMANCE CHARACTERISTICS

##### Analytical Sensitivity

The analytical sensitivity of the Free T3 EIA Test Kit is less than 0.8 pg/mL.

##### Accuracy

The Free T3 EIA Test Kit has been compared to a leading commercial Free T3 EIA test using clinical specimens. A total of 143 clinical specimens ranging from 1.87-21.84pg/mL were run and analyzed using least square regression analysis. The results show that the Free T3 EIA Test Kit has good correlation with the reference method.

Method	Equation	Correlation
ACON "x" Reference "y"	y=1.011x-0.509	0.954

##### Reproducibility

**Intra-Assay:** Within-run precision has been determined by using 20 replicates of three specimens respectively containing low, middle and high concentration of Free T3.

**Inter-Assay:** Between-run precision has been determined by using 2 replicates of three specimens respectively containing low, middle and high concentration of Free T3 for 10 times over a 5-day period.

Coefficient of Variation (%)	
Intra-Assay	Inter-Assay
<15%	<15%

##### Interferences

No interference was observed in specimens containing the substances in the below table:

Substance	Concentration	Substance	Concentration
Caffeine	0.012 mg/mL	Salicylic acid	0.2 mg/mL
Bilirubin	2 mg/mL	Ascorbic acid	0.04 mg/mL

The determined concentration of Free T3 may increase when specimens containing the substances in the below table:

Substance	Concentration	Substance	Concentration
Ibuprofen	0.12 mg/mL	Triglyceride	5 mg/mL
Paracetamol	0.1 mg/mL	/	/

The determined concentration of free T3 may decrease when specimens containing the substances in the below table:

Substance	Concentration	Substance	Concentration
Albumin	75 mg/mL	Cholesterol	2 mg/mL
Hemoglobin	10 mg/mL	/	/

##### Cross-Reactivity

T3 analogues were spiked in human serum (without Free T3) at certain concentrations and tested with the Free T3 EIA Test kit. The corresponding Free T3 concentration with the same absorbance was determined based on the calibration curve.

Substance	Spiked concentration	Determined concentration	Cross reactivity
Thyroxine	10ug/ml	9.9 pg/mL	<0.0001%
3,5-diiodo-L-tyrosine	10ug/ml	2.1 pg/mL	<0.0001%
Tyrosine	10ug/ml	38.5 pg/mL	<0.001%
3,3',5-triiodothyroacetic acid	1ng/ml	9.4 pg/mL	0.94%

#### BIBLIOGRAPHY

- O'Neill, MJ, editor. *The Merck Index*. 13th ed. Whitehouse Station, NJ. Merck & Co., Inc. (2001), 987-988.
- Larson, PR. *Triiodothyronine: Review of Recent Studies of its Physiology and Pathophysiology in Man*. Metabolism. (1972), 21:1073-1092.
- S Utiger, RD. *Serum triiodothyronine in Man*. Annual Review of Medicine. (1974), 25:289-302.
- Hamburger, JI. *Evolution of Toxicity in Solitary Nontoxic Autonomously Functioning Thyroid Nodules*. J. Clin. Endocrinol. Metab. (1980), 50:1089.
- Ladenson, PW. *Diagnosis of Thyrotoxicosis*. In: Braverman, LE, Utiger, RD, editors. The Thyroid. 7th Ed (1996) 708-712.

#### Index of Symbols

	Consult instructions for use		Tests per kit		Manufacturer
	For <i>in vitro</i> diagnostic use only		Use by		Authorized Representative
	Catalog #		Lot Number		Store between 2-8°C
	Free T3		Substrate A		Substrate B
	Wash Buffer (25x)		Conjugate (11x)		Calibrator 1
	Calibrator 2		Calibrator 3		Calibrator 4
	Calibrator 5		Calibrator 6		Conjugate Diluent
	Microwell Plate		Stop Solution		Package Insert
	Plate Sealer				

**ACON Laboratories, Inc.**  
10125 Mesa Rim Road  
San Diego, CA 92121, USA

**MDSS GmbH**  
Schiffgraben 41  
30175 Hannover, Germany

Number: 1150551503  
Effective date: 2017-01-26